



**ELECTRONICS
DIVISION**

**Model 483C15
MANUAL 483C05 SERIES
Installation and Operating Manual**

**For assistance with the operation of this product , contact the Division of PCB
Piezotronics, Inc.**

Division toll-free 888-684-0015

24-hour SensorLineSM 716-684-0001

Fax 716-684-0987

E-mail electronics@pcb.com



 **PCB** *PIEZOTRONICS*^{INC.}
ELECTRONICS DIVISION

The information contained in this document supersedes all similar information that may be found elsewhere in this manual.

Total Customer Satisfaction – PCB Piezotronics guarantees Total Customer Satisfaction. If, at any time, for any reason, you are not completely satisfied with any PCB product, PCB will repair, replace, or exchange it at no charge. You may also choose to have your purchase price refunded in lieu of the repair, replacement, or exchange of the product.

Service – Due to the sophisticated nature of the sensors and associated instrumentation provided by PCB Piezotronics, user servicing or repair is not recommended and, if attempted, may void the factory warranty. Routine maintenance, such as the cleaning of electrical connectors, housings, and mounting surfaces with solutions and techniques that will not harm the physical material of construction, is acceptable. Caution should be observed to insure that liquids are not permitted to migrate into devices that are not hermetically sealed. Such devices should only be wiped with a dampened cloth and never submerged or have liquids poured upon them.

Repair – In the event that equipment becomes damaged or ceases to operate, arrangements should be made to return the equipment to PCB Piezotronics for repair. User servicing or repair is not recommended and, if attempted, may void the factory warranty.

Calibration – Routine calibration of sensors and associated instrumentation is

recommended as this helps build confidence in measurement accuracy and acquired data. Equipment calibration cycles are typically established by the users own quality regimen. When in doubt about a calibration cycle, a good “rule of thumb” is to recalibrate on an annual basis. It is also good practice to recalibrate after exposure to any severe temperature extreme, shock, load, or other environmental influence, or prior to any critical test.

PCB Piezotronics maintains an ISO-9001 certified metrology laboratory and offers calibration services, which are accredited by A2LA to ISO/IEC 17025, with full traceability to N.I.S.T. In addition to the normally supplied calibration, special testing is also available, such as: sensitivity at elevated or cryogenic temperatures, phase response, extended high or low frequency response, extended range, leak testing, hydrostatic pressure testing, and others. For information on standard recalibration services or special testing, contact your local PCB Piezotronics distributor, sales representative, or factory customer service representative.

Returning Equipment – *Following these procedures will insure that your returned materials are handled in the most expedient manner.* Before returning any equipment to PCB Piezotronics, contact your local distributor, sales representative, or factory customer service representative to obtain a Return

Materials Authorization (RMA) Number. This RMA number should be clearly marked on the outside of all package(s) and on the packing list(s) accompanying the shipment. A detailed account of the nature of the problem(s) being experienced with the equipment should also be included inside the package(s) containing any returned materials.


A Purchase Order, included with the returned materials, will expedite the turn-around of serviced equipment. It is recommended to include authorization on the Purchase Order for PCB to proceed with any repairs, as long as they do not exceed 50% of the replacement cost of the returned item(s). PCB will provide a price quotation or replacement recommendation for any item whose repair costs would exceed 50% of replacement cost, or any item that is not economically feasible to repair. For routine calibration services, the Purchase Order should include authorization to proceed and return at current pricing, which can be obtained from a factory customer service representative.

Warranty – All equipment and repair services provided by PCB Piezotronics, Inc. are covered by a limited warranty against defective material and workmanship for a period of one year from date of original purchase. Contact

PCB for a complete statement of our warranty. Expendable items, such as batteries and mounting hardware, are not covered by warranty. Mechanical damage to equipment due to improper use is not covered by warranty. Electronic circuitry failure caused by the introduction of unregulated or improper excitation power or electrostatic discharge is not covered by warranty.

Contact Information – International customers should direct all inquiries to their local distributor or sales office. A complete list of distributors and offices can be found at www.pcb.com. Customers within the United States may contact their local sales representative or a factory customer service representative. A complete list of sales representatives can be found at www.pcb.com. Toll-free telephone numbers for a factory customer service representative, in the division responsible for this product, can be found on the title page at the front of this manual. Our ship to address and general contact numbers are:

PCB Piezotronics, Inc.
3425 Walden Ave.
Depew, NY 14043 USA
Toll-free: (800) 828-8840
24-hour SensorLineSM: (716) 684-0001
Website: www.pcb.com
E-mail: info@pcb.com

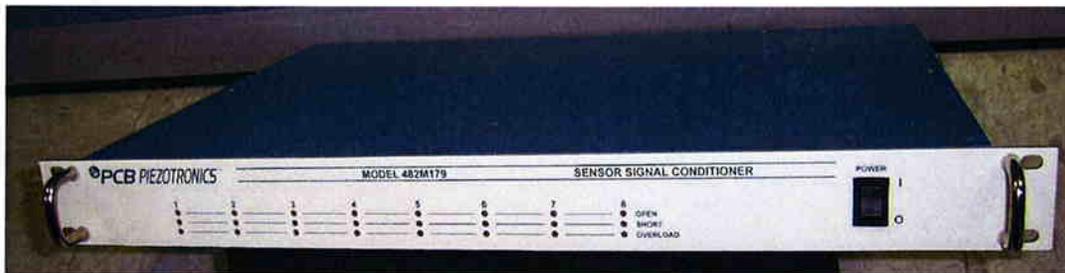

SIGNAL CONDITIONER

Models 483C05/483C15

GENERAL OPERATION MANUAL

For powering ICP[®] sensors and in-line charge converters, this signal conditioner provides a cost effective method for powering large numbers of sensor channels.

The 483C Series is available with many different options from PCB. This manual describes the functions of the most economical signal conditioner with unity gain (483C05) and x1, x10, x100 jumper selectable gain (483C15), of that series.



PCB PIEZOTRONICS, INC. 3425 WALDEN AVENUE DEPEW, NY 14043-2495 PHONE 716-684-0001 FAX 716-684-0987

[®]ICP is a registered trademark of PCB Group, Inc.

KS398

Table of Contents

Table of Contents	i
1-1. Introduction	1
1-2. Safety Considerations	1
1-3. Equipment Rating	2
1-4. Model 483C15 System Description	2
1-5. Model 483C05 System Description	4
1-6. Installation	4
1-7. Grounding Techniques	4
1-8. Unit Power	5
1-9. Maintenance and Repair	5
Appendix	
Specification Sheet	
Outline Drawing	

Manual Number: 38548
Manual Revision: NR
ECO Number:

1-1. Introduction

The Model 483C05 is a basic ICP[®] signal conditioner that provides an adjustable current source to drive ICP[®] sensors. Additionally it has Open, Short and Overload Input fault condition indicators.

The Model 483C15 is an ICP[®] signal conditioner that has all the features of the 483C05 plus jumper selectable (x1, x10, and x100) Gain options and an Overload range selection. An easy to open cover, allows access to the jumper selections.

The following sections describe these devices in more detail.

1-2. Safety Considerations

WARNING SYMBOLS AND TERMS

The following symbols and terms may be found on the equipment described in this manual.



This symbol on the unit indicates that the user should refer to the operating instructions located in the manual.



This symbol on the unit indicates that high voltage may be present. Use standard safety precautions to avoid personal contact with this voltage.



This symbol indicates that the test fixture, Model 483C15/483C05, must be connected to earth ground via the power cord.

The **WARNING** heading used in this manual explains dangers that might result in personal injury or death. Always read the associated information very carefully before performing the indicated procedure.

The **CAUTION** heading used in this manual explains hazards that could damage the instrument.

WARNING 1: *The power supply/signal conditioner should not be opened by anyone other than qualified service personnel.* This product is intended for service by qualified personnel who recognize shock hazards and are familiar with the safety precautions required to avoid injury.

WARNING 2: This equipment is designed with user safety in mind; however, the protection provided by the equipment may be impaired if the equipment is used in a manner not specified by PCB Piezotronics, Inc.

CAUTION 1: *Cables can kill your equipment.* High voltage ElectroStatic Discharge (ESD) can damage electrical devices. Similar to a capacitor, a cable can hold a charge caused by triboelectric transfer, such as that which occurs in the following:

- Laying on and moving across a rug.
- Any movement through air.
- The action of rolling out a cable.
- Contact to a non-grounded person

The solution for product safety: 1) Connect the cables only with the AC power off. 2) Temporarily “short” the end of the cable before attaching it to any signal input or output.

CAUTION 2: *ESD considerations should be made prior to performing any internal adjustments on the equipment.* Any piece of electronic equipment is vulnerable to ESD when opened for adjustments. Internal adjustments should therefore be done **ONLY** at an ESD-safe work area. Many products have ESD protection, but the level of protection may be exceeded by extremely high voltage that is typically present in normal situations.

1-3. Equipment Rating

For complete specifications, please refer to the enclosed Specification Sheet. This equipment operates optimally at +32 to +120°F (0 to +50°C), in an environment having <85% relative humidity. Its line power frequency range is 47-63 Hz.

The 483C15/483C05 devices require 100-240 VAC with 0.7A to operate. In turn, they supply 26 VDC @ 2 to 20 mA excitation voltage to connected ICP® sensors or in-line charge converters. The units get power via Standard IEC AC power cord PCB Model 017AXX.

1-4. Model 482C15 System Description

The Model 483C15 is a eight channel signal conditioning rack mount unit designed to interface measurement signals to readout or recording devices.

The following are features that come standard on 483C15 units:

- Input fault and overload LED's with jumper selectable overload level of +/-5V or +/-10V
- Variable ICP® source current, 0 to 20 mA
- Jumper selectable Voltage input mode
- Jumper selectable gain of x1, x10, x100 (483C15 Only)
- Lighted power indicator on the front panel
- Rear panel BNC input/output connectors
- Optional L.P. plug in filters (477A series type) various 2-pole frequencies avail. Consult factory
- Rack mountable enclosure.

1-4.1. Model 483C15 ICP® Input/Output Mode

The Model 483C15 contains a regulated 26 VDC power supply that provides constant current for up to 8 individual channels. Both the output and input connections utilize BNC connectors and are brought out through the rear panel. The unit is AC coupled only. The 482C series offers optional DC Coupling. Consult factory

1-4.2. Adjusting the Current Source

The Current adjustments are located on the rear of the unit. Use a standard small flat screwdriver to adjust the "I ADJ" potentiometers. Turning the adjustment slot clockwise will increase the current, while counterclockwise will decrease the current. Do this adjustment only while a DC mA meter or DMM set to mA is connected to any of the group of 4 "ICP" BNC's. One adjustment controls 4 channels. The unit is factory set to 4mA and can be adjusted between 0mA-20mA.


1-4.3. Fault Indications

The three red LED's on the front panel are all indicators of some type of problem. The normal good operation state is when all fault lights are off. The "OPEN" light indicates that the Bias voltage is over that of most sensors and is close to an open circuit voltage of 26VDC. The "SHORT" light indicates a very low Bias voltage close to 0VDC. The

“OVERLOAD” light indicates a signal level of +/-10V Peak has been detected and the signal may be in danger of clipping. These fault lights are active for all channels, at the same time.

1-4.4. Gain selection / Jumper definition

The 483C15 has internal jumpers that are accessed by opening the top cover. Remove all the Phillips screws, allowing the cover to be opened. The various jumpers are all labeled on the PC Boards. Each channel can be set to your selected gain and other options. The selection of all these features with jumpers allows the 483C15 to have the functionality of many other higher priced units. See the table that explains the function and number of each jumper. Place the blue jumpers in various locations as shown below.

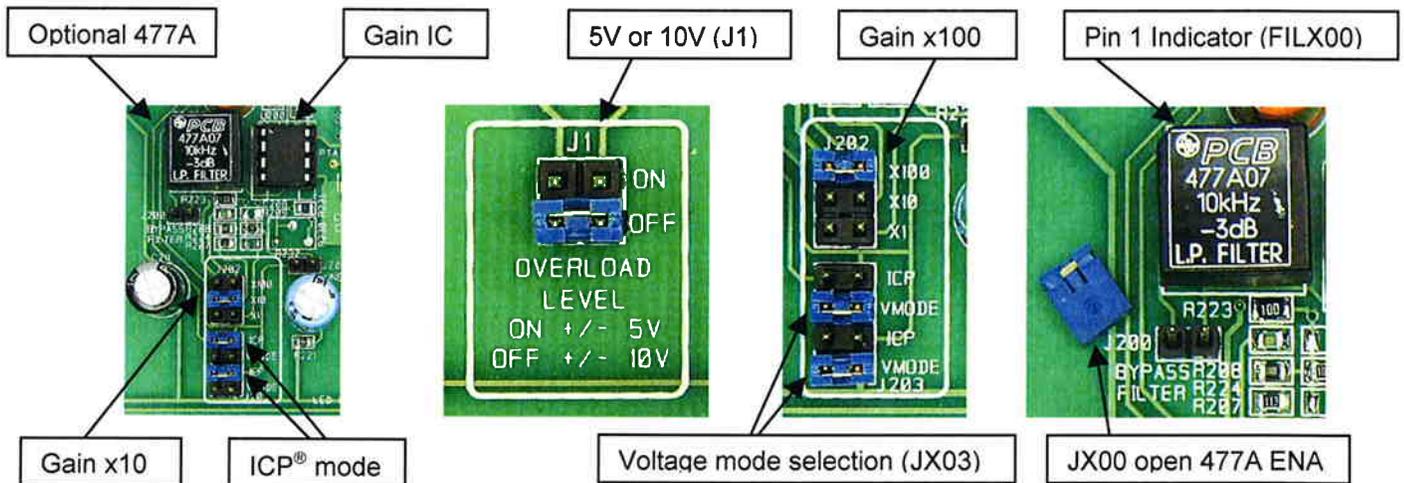

. “X” represents channel number on each bd. Channels 5-8 are controlled by the bd. on the right side of the unit.

Gain 1 10 100	JX02	1 jumper per channel
Overload 5V/10V	J1	Controls all channels
Voltage Mode	JX03	2 jumpers per channel
Bypass Filter	JX00	Remove to install filter module
477A Filter	FILX00	Install filter here per channel

1-5. Model 483C05 System Description

The Model 483C05 is a basic eight channel signal conditioning rack mount unit designed to interface measurement signals to readout or recording devices.

The following are features that come standard on every 483C05:

- Unity gain
- Input fault and overload LED's
- Variable ICP® source current, 0 to 20 mA
- Lighted power indicator on the front panel
- Rear panel BNC input/output connectors
- Rack mountable enclosure.

1-5.1. Model 483C05 ICP® Input/Output Mode

The Model 483C05 contains a regulated 26 VDC power supply that provides constant current for up to 8 individual channels. Both the output and input connections utilize BNC connectors and are brought out through the rear panel. The unit is AC coupled only. The 482C series offers optional DC Coupling. Consult factory

1-5.2. Adjusting the Current Source

The Current adjustments are located on the rear of the unit. Use a standard small flat screwdriver to adjust the "I ADJ" potentiometers. Turning the adjustment slot clockwise will increase the current, while counterclockwise will decrease the current. Do this adjustment only while a DC mA meter or DMM set to mA is connected to any of the group of 4 "ICP" BNC's. One adjustment controls 4 channels. The unit is factory set to 4mA and can be adjusted between 0mA-20mA.

1-5.3. Fault Indications

The three red LED's on the front panel are all indicators of some type of problem. The normal good operation state is when all fault lights are off. The "OPEN" light indicates that the Bias voltage is over that of most sensors and is close to an open circuit voltage of 26VDC. The "SHORT" light indicates a very low Bias voltage close to 0VDC. The "OVERLOAD" light indicates a signal level of +/-10V Peak has been detected and the signal may be in danger of clipping. These fault lights are active for all channels, at the same time.

1-6. Installation

Both the Model 483C15 and the Model 483C05 come packaged in a standard 19" 1U rack mount enclosure and require very little in term of installation. The box should be located in such a way as to allow convenient access to the power outlet for disconnect purposes. Since these units have low power consumption, they can be located in confined environments.

NOTE: Specific installation is available; contact PCB

1-7. Grounding Techniques

Integrating either of these Models into an application that links the outputs to other test equipment powered by line voltages may lead to errors or loss of signal-to-noise ratio due to ground loops. The evidence of ground loops is easily seen whenever the fundamental frequency (50 or 60 Hz) or a multiple of the fundamental frequency is present in the system when the sensors are “at rest.” In order to maintain the operating specification of noise and reduce the effects of line interference, proper grounding techniques should be used. The following procedure may be helpful:

1. Make sure the signal ground lines of all equipment are tied together. The signal grounds of the channels are typically tied together via the case of the input and output BNC connectors. The individual channels of the Model 483C15 and 483C05 have their signal ground line tied together internally at the power supply.
2. Insure that the sensor does not pick up line noise from the body under test. The case of the sensor should be isolated from the body under (ground) using an isolation pad. The isolation pad breaks the loop formed by the signal path of the sensor to the unit and the return (ground) from the unit back to the sensor.
3. Make sure that all equipment signal grounds of the test system are tied to the Earth ground at a single point and the connections linking the equipment ground are made using a wire that can provide a very low impedance connection.

1-8. Unit Power

1-8.1. Power: Standard AC Line power

Plug the unit into any 100-240VAC 47-63Hz power source, attach the supplied ferrite clamp on the AC cord to ensure CE conformance, and press the “ON/OFF” – “IN/OUT” switch.

CAUTION 3: Refer to the rear panel for proper input voltage. Standard IEC 320 input connector with internal fuse.

1-9. Maintenance and Repair

It is not recommended that the customer attempt repairs of the Model 483C15 or 483C05. Should trouble occur, contact the factory for assistance.

Performance
Channels 8
Sensor Input Type(s) ICP®, Voltage [2]
Voltage Gain(± 1 %)(at 500 Hz) x1, x10, x100 [2]
Output Range(Maximum) ± 10 V
Frequency Range(-3 dB) 0.05 to 50,000 Hz [4]
Phase Response(at 1 kHz) ± 1°
Cross Talk(maximum) -72 dB
Fault/Bias Monitor/Meter(LED) Open/Short/Overload

Environmental
Temperature Range(Operating) +32 to +120 °F
Temperature Range(Storage) 0 to +50 °C

Electrical
Power Required AC Power
AC Power(47 to 63 Hz) 100 to 240 VAC
AC Power ≤ 0.7 amps
Excitation Voltage(± 1 VDC)(To Sensor) +26 VDC
Constant Current Excitation(To Sensor) 0 to 20 mA
DC Offset <20 mV

Output Impedance 50 ohm
Overload Threshold(± 1.0 Vpk) +10/+5 Vpk
Broadband Electrical Noise(1 to 10,000 Hz)(Gain x1) 5.6 µV rms
Spectral Noise(1 Hz) 0.67 µV/√Hz
Spectral Noise(10 Hz) 0.10 µV/√Hz
Spectral Noise(100 Hz) 0.06 µV/√Hz
Spectral Noise(1 kHz) 0.06 µV/√Hz
Spectral Noise(10 kHz) 0.05 µV/√Hz

Broadband Electrical Noise(1 to 10,000 Hz)(Gain x10) 21 µV/rms
Spectral Noise(1 Hz) 5.10 µV/√Hz
Spectral Noise(10 Hz) 0.60 µV/√Hz
Spectral Noise(100 Hz) 0.22 µV/√Hz
Spectral Noise(1 kHz) 0.22 µV/√Hz
Spectral Noise(10 kHz) 0.19 µV/√Hz

Broadband Electrical Noise(1 to 10,000 Hz)(Gain x100) 165 µV/rms
Spectral Noise(1 Hz) 57 µV/√Hz
Spectral Noise(10 Hz) 5.2 µV/√Hz
Spectral Noise(100 Hz) 1.7 µV/√Hz
Spectral Noise(1 kHz) 1.8 µV/√Hz
Spectral Noise(10 kHz) 1.4 µV/√Hz

Physical
Electrical Connector(ICP® Sensor Input) BNC Jack
Electrical Connector(Output) BNC Jack
Electrical Connector(AC Power Input) IEC 320
Size (Height x Width x Depth) 1.75 in x 1.9 in x 13.5 in 43.7 cm x 48.26 mm x 343 mm
Weight 6.25 lb 2.83 kg

OPTIONAL VERSIONS
Optional versions have identical specifications and accessories as listed for the standard model except where noted below. More than one option may be used.

NOTES:
[1] User adjustable, factory set at 4 mA (± 0.5 mA). Each control adjusts 4 channels.
[2] Jumper selectable on internal circuit board.
[3] Typical.
[4] Unfiltered response frequency may be limited by low pass plug-in filter (PCB Model 477A)
[5] See PCB Declaration of Conformance PS024 for details.

SUPPLIED ACCESSORIES:
Model 017AXX Power Cord (1)

Entered: H.S. Engineer: P.A.H. Sales: J.D.M. Approved: J.P.V. Spec Number: 38622
Date: 9/18/07 Date: 9/18/07 Date: 9/18/07

PCB PIEZOTRONICS™
ELECTRONICS DIVISION
3425 Walden Avenue, Depew, NY 14043
Phone: 716-684-0001
Fax: 716-684-0987
E-Mail: electronics@pcb.com

CE [5]
All specifications are at room temperature unless otherwise specified.
In the interest of constant product improvement, we reserve the right to change specifications without notice.
ICP® is a registered trademark of PCB Group, Inc.

PCB Piezotronics Inc. claims proprietary rights in the information disclosed herein. Neither it nor any reproduction thereof will be disclosed to others without the written consent of PCB Piezotronics Inc.




38442

REVISIONS

REV	DESCRIPTION	ECH	APPD
NR	RELEASED TO DRAFTING		EB 9/5/07

EXTERNAL AC POWER INPUT

16X BNC CONNECTORS

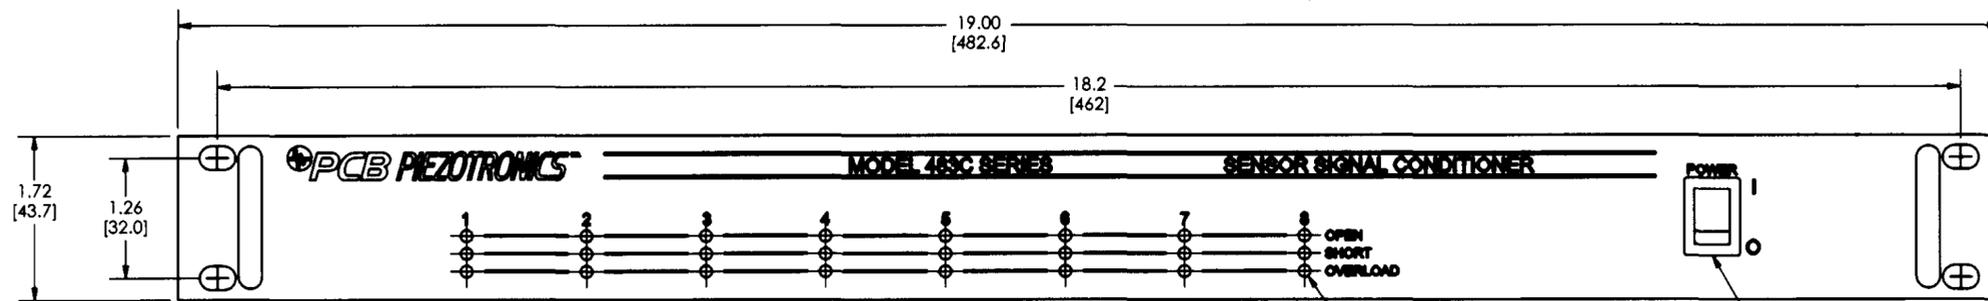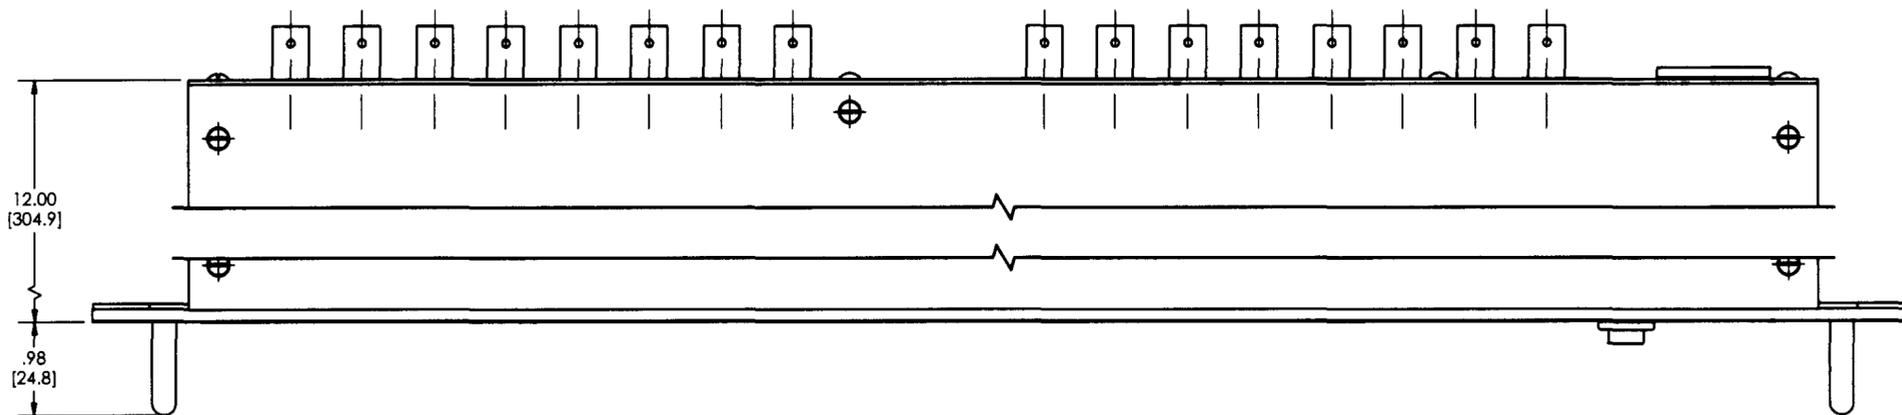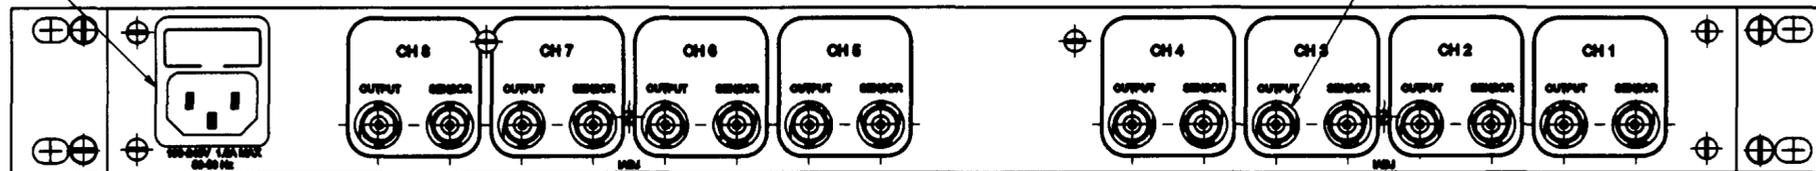

(RED) LED'S

AC POWER SWITCH

UNLESS OTHERWISE SPECIFIED TOLERANCES ARE:		<table border="1"> <tr> <td>DRAWN</td> <td>MDI</td> <td>8/31/07</td> <td>MPG</td> <td>89.0</td> <td>9/5/07</td> </tr> <tr> <td>CHE'D</td> <td>EB</td> <td>9/5/07</td> <td>ENGR</td> <td>AP</td> <td>9/5/07</td> </tr> <tr> <td>APP'D</td> <td>MP</td> <td>9/5/07</td> <td>SALES</td> <td>AP</td> <td>9/5/07</td> </tr> </table>	DRAWN	MDI	8/31/07	MPG	89.0	9/5/07	CHE'D	EB	9/5/07	ENGR	AP	9/5/07	APP'D	MP	9/5/07	SALES	AP	9/5/07	<p>3425 WALDEN AVE. DEPEW, NY 14043 (716) 684-0001 E-MAIL: sales@pcb.com</p>		
DRAWN	MDI	8/31/07	MPG	89.0	9/5/07																		
CHE'D	EB	9/5/07	ENGR	AP	9/5/07																		
APP'D	MP	9/5/07	SALES	AP	9/5/07																		
DIMENSIONS IN INCHES	DIMENSIONS IN MILLIMETERS [IN BRACKETS]	<table border="1"> <tr> <td>DECIMALS</td> <td>XX ± .03</td> <td>DECIMALS</td> <td>X ± 0.8</td> </tr> <tr> <td></td> <td>XXX ± .010</td> <td></td> <td>XX ± 0.25</td> </tr> <tr> <td>ANGLES</td> <td>± 2 DEGREES</td> <td>ANGLES</td> <td>± 2 DEGREES</td> </tr> <tr> <td>FILLETS AND RADII</td> <td>.003 - .006</td> <td>FILLETS AND RADII</td> <td>[0.07 - 0.13]</td> </tr> </table>	DECIMALS	XX ± .03	DECIMALS	X ± 0.8		XXX ± .010		XX ± 0.25	ANGLES	± 2 DEGREES	ANGLES	± 2 DEGREES	FILLETS AND RADII	.003 - .006	FILLETS AND RADII	[0.07 - 0.13]	<table border="1"> <tr> <td>CODE IDENT. NO.</td> <td>DWG. NO.</td> </tr> <tr> <td>52681</td> <td>38442</td> </tr> </table>	CODE IDENT. NO.	DWG. NO.	52681	38442
DECIMALS	XX ± .03	DECIMALS	X ± 0.8																				
	XXX ± .010		XX ± 0.25																				
ANGLES	± 2 DEGREES	ANGLES	± 2 DEGREES																				
FILLETS AND RADII	.003 - .006	FILLETS AND RADII	[0.07 - 0.13]																				
CODE IDENT. NO.	DWG. NO.																						
52681	38442																						
		<p>OUTLINE DRAWING MODEL 483C05/15 SENSOR SIGNAL CONDITIONER</p>		<p>SCALE: .75X SHEET 1 OF 1</p>																			